


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2025, Rack A, Plate 1, Well B08, 171599  
[9822856DEE775115] Dec 23, 2025 11:41:23 Pressure = 77 bar (76 to 79)

FA

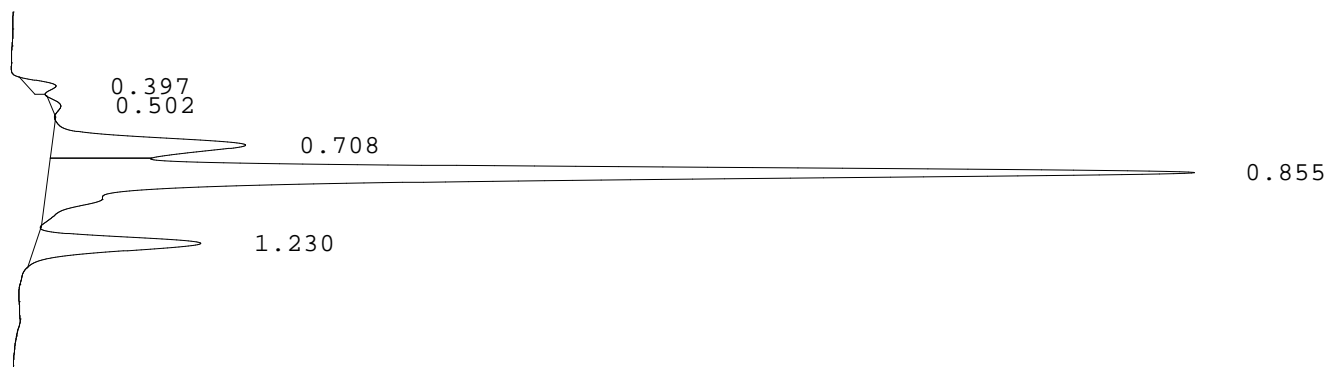

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.397	F 0.47	1.3%	8946	
2	0.502	F 0.59	0.5%	3554	
3	0.708	F 0.83	14.9%	100804	Acetylated F peak
4	0.855	F 1.01	72.8%	493955	Consistent with F
5	1.230	A 1.02	10.5%	71410	A peak
Total Area:				678669	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range