


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2022, Rack A, Plate 1, Well B05, 171532
 [8C36958675082660] Dec 19, 2025 10:38:15 Pressure = 76 bar (76 to 78)

FA

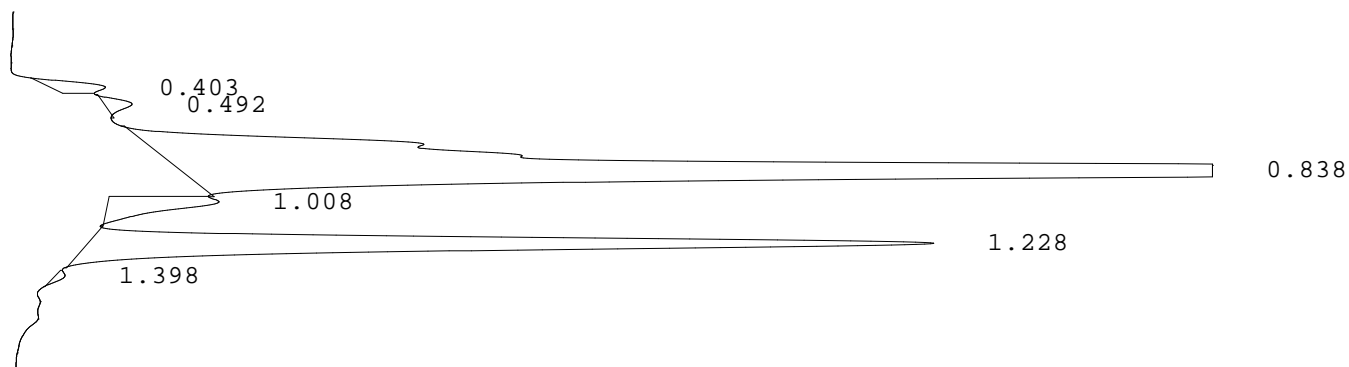

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.48	1.1%	16666	
2	0.492	F 0.58	0.6%	9726	
3	0.838	F 0.99	72.6%	1087051	Consistent with F
4	1.008	F 1.19	3.3%	49747	
5	1.228	A 1.02	22.1%	331498	A peak - REVIEW
6	1.398	S 0.89	0.2%	3176	
Total Area:				1497864	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range