


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2031, Rack A, Plate 1, Well A01, 484138-P
[C923C7BAED75711F] Dec 30, 2025 08:45:20 Pressure = 77 bar (77 to 79)

FA

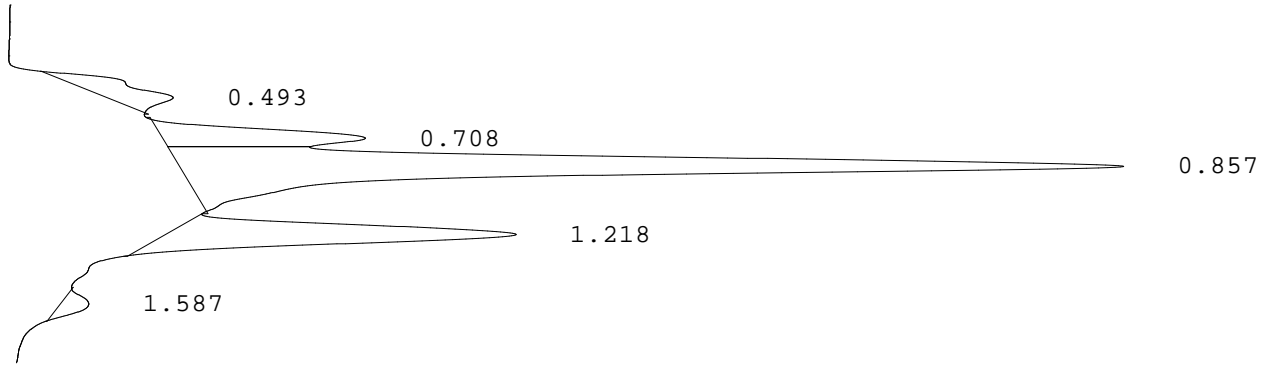

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.493	F 0.58	5.7%	52393	
2	0.708	F 0.83	10.8%	99484	Acetylated F peak
3	0.857	F 1.01	60.1%	553233	Consistent with F
4	1.218	A 1.01	21.6%	198770	A peak - REVIEW
5	1.587	S 1.01	1.8%	16636	4 3

Total Area: 920516

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range