


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1884, Rack A, Plate 1, Well B10, 457246
 [DD353715D4AEDBB5] Aug 13, 2025 11:25:51 Pressure = 60 bar (60 to 61)

FA

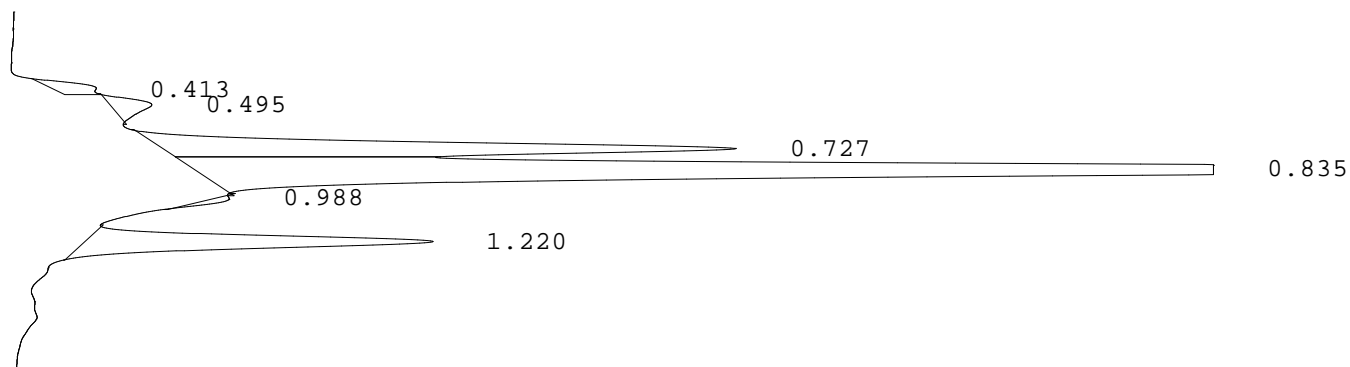

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.413	F 0.49	1.5%	15180	
2	0.495	F 0.59	1.9%	19578	
3	0.727	F 0.87	20.5%	214134	
4	0.835	F 1.00	62.6%	654429	Consistent with F
5	0.988	F 1.18	0.7%	7283	
6	1.220	A 1.01	12.9%	134574	A peak
Total Area:				1045178	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range