


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2025, Rack A, Plate 1, Well E03, 490113 FA
 [DC22C538B9282CEA] Dec 23, 2025 12:46:04 Pressure = 75 bar (75 to 77)

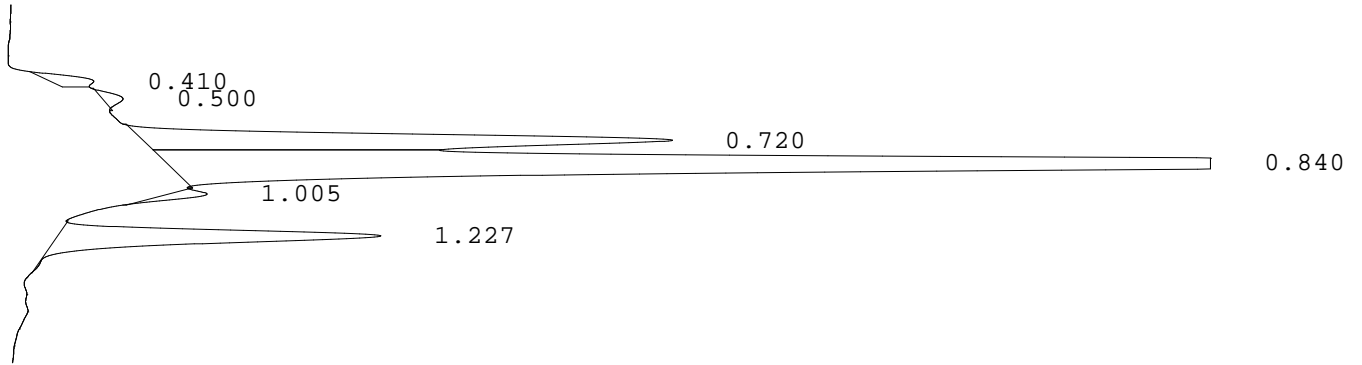

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.48	1.2%	13769	
2	0.500	F 0.59	0.7%	7860	
3	0.720	F 0.85	19.0%	210666	Acetylated F peak
4	0.840	F 0.99	66.4%	736586	Consistent with F
5	1.005	F 1.18	1.1%	12185	
6	1.227	A 1.01	11.6%	128869	A peak
Total Area:				1109935	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range