


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2025, Rack A, Plate 1, Well D12, 486853
 [8836D538B900A44A] Dec 23, 2025 12:40:00 Pressure = 75 bar (75 to 77)

FA

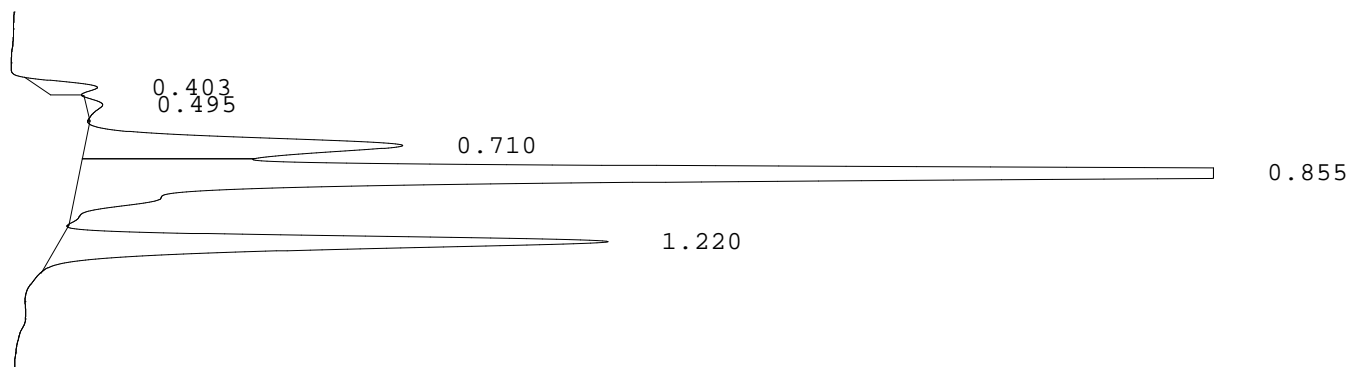

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	1.6%	19173	
2	0.495	F 0.58	0.5%	6554	
3	0.710	F 0.83	14.2%	169725	Acetylated F peak
4	0.855	F 1.00	64.5%	773034	Consistent with F
5	1.220	A 1.00	19.1%	229119	A peak
				Total Area: 1197605	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range