


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1974, Rack A, Plate 1, Well C10, 478842
 [C877E3EE67F0AC68] Nov 11, 2025 12:18:13 Pressure = 66 bar (66 to 68)

FA

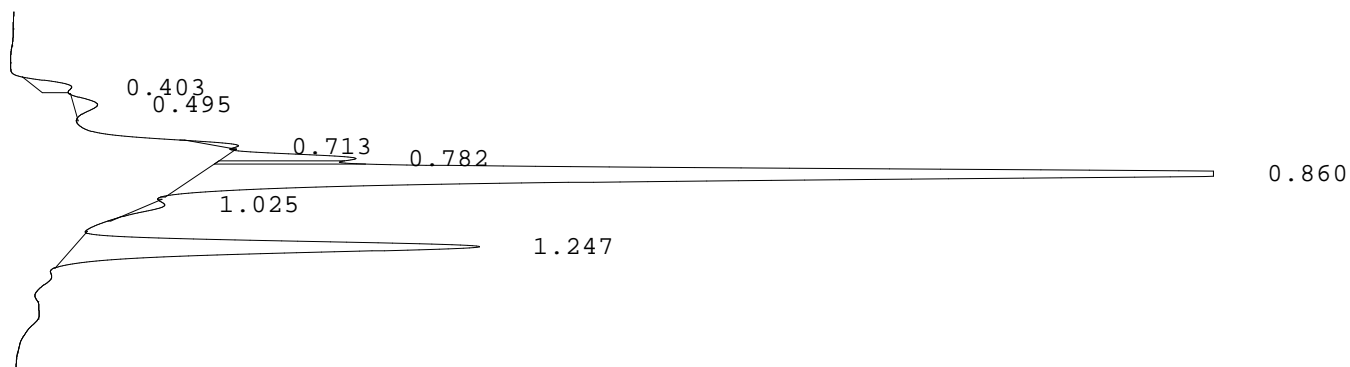

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	1.8%	11676	
2	0.495	F 0.57	1.5%	9643	
3	0.713	F 0.82	0.8%	4999	
4	0.782	F 0.90	5.8%	38205	
5	0.860	F 0.99	66.1%	437835	Consistent with F
6	1.025	F 1.18	1.0%	6774	
7	1.247	A 1.01	23.1%	153075	A peak - REVIEW
Total Area:				662207	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range