


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2022, Rack A, Plate 1, Well A05, 482093  
 [CD27D486778084CA] Dec 19, 2025 10:14:00 Pressure = 76 bar (75 to 78)

FA

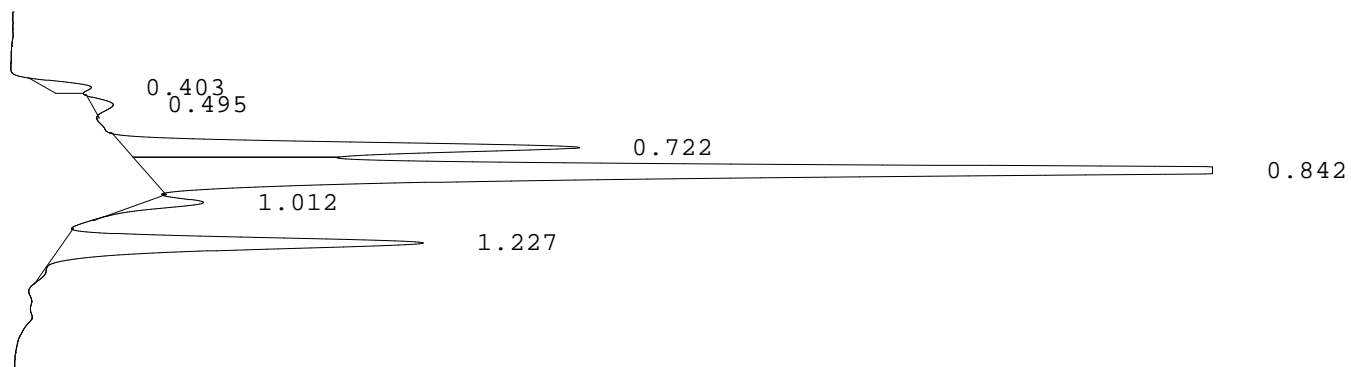

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.48	1.6%	14077	
2	0.495	F 0.58	0.9%	8029	
3	0.722	F 0.85	18.4%	164532	
4	0.842	F 0.99	61.3%	547559	Consistent with F
5	1.012	F 1.19	2.2%	19281	
6	1.227	A 1.02	15.6%	139485	A peak
Total Area:				892963	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range