


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 1993, Rack A, Plate 1, Well E11, 458148  
 [DC36AC87A2CFD315] Nov 25, 2025 12:34:27 Pressure = 68 bar (67 to 69)

FA

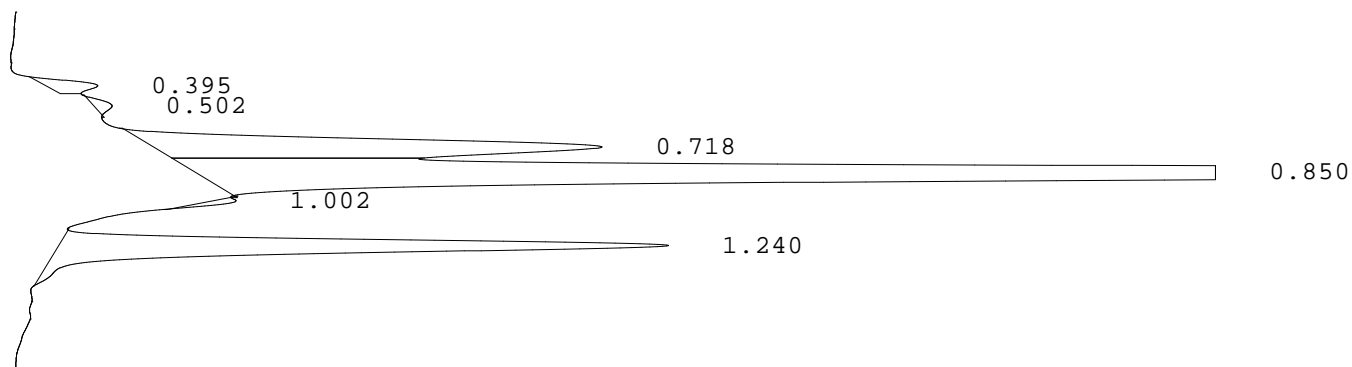

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.395	F 0.46	1.2%	16363	
2	0.502	F 0.58	0.5%	6950	
3	0.718	F 0.83	15.9%	223915	Acetylated F peak
4	0.850	F 0.99	64.1%	903880	Consistent with F
5	1.002	F 1.16	0.5%	7628	
6	1.240	A 1.01	17.8%	251385	A peak
Total Area:				1410121	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range