


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2022, Rack A, Plate 1, Well A10, 484366  
 [DD33848677A20C60] Dec 19, 2025 10:24:07 Pressure = 76 bar (75 to 77)

FA

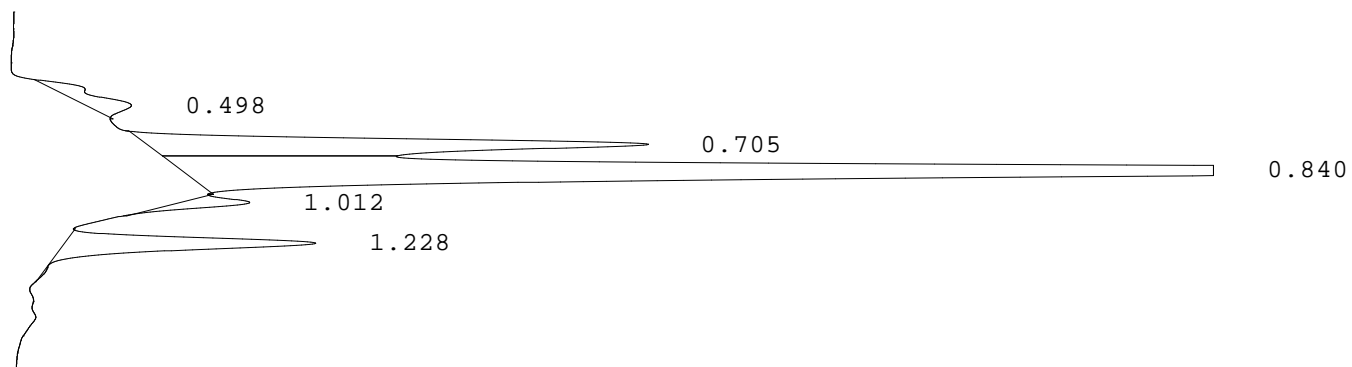

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.498	F 0.59	3.0%	30970	
2	0.705	F 0.83	19.4%	200092	Acetylated F peak
3	0.840	F 0.99	66.2%	682473	Consistent with F
4	1.012	F 1.19	2.1%	21840	
5	1.228	A 1.02	9.3%	95937	A peak
				Total Area: 1031312	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range