


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2029, Rack A, Plate 1, Well H02, 490093  
[9962D3EDEFFFF31D] Dec 29, 2025 13:48:01 Pressure = 74 bar (73 to 75)

FA

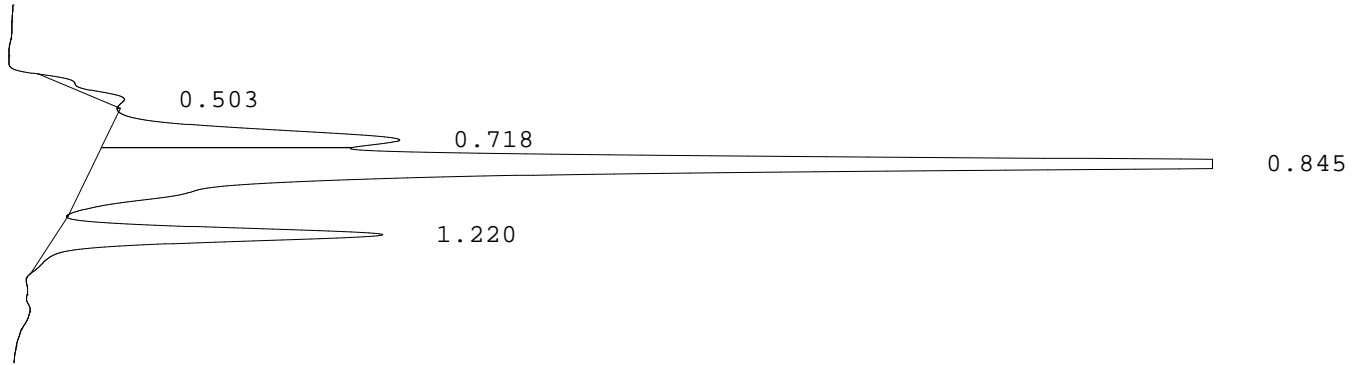

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.503	F 0.59	1.5%	16474	
2	0.718	F 0.84	14.4%	158637	Acetylated F peak
3	0.845	F 0.98	71.0%	784652	Consistent with F
4	1.220	A 1.01	13.1%	144619	A peak
Total Area:				1104382	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range