


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2022, Rack A, Plate 1, Well H12, 490103  
 [9D6294C2DD8A04E0] Dec 19, 2025 13:23:59 Pressure = 73 bar (72 to 75)

FA

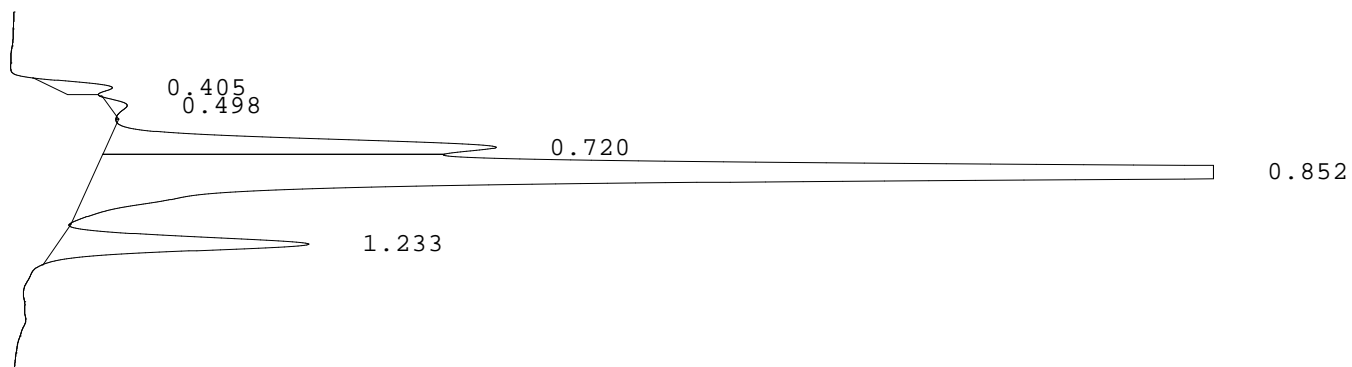

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	1.4%	19081	
2	0.498	F 0.58	0.5%	7086	
3	0.720	F 0.84	13.3%	179179	Acetylated F peak
4	0.852	F 0.99	76.5%	1031436	Consistent with F
5	1.233	A 1.01	8.3%	111411	A peak
Total Area:				1348193	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range