


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2204, Rack A, Plate 1, Well A06, 487179
[DD3888AC104866C8] Jul 23, 2026 10:21:13 Pressure = 92 bar (92 to 94)

FA

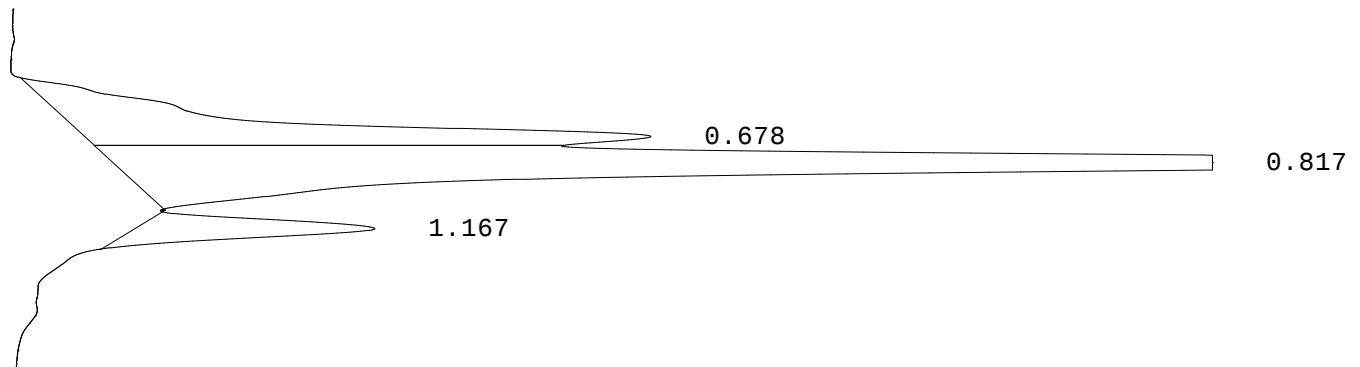

PEAK	RT	REL	RT	% CONC	AREA	COMMENT
1	0.678	F	0.82	25.4%	410607	
2	0.817	F	0.99	66.5%	1075983	Consistent with F
3	1.167	A	1.01	8.1%	130357	A peak
Total Area: 1616947						

Codes: 1) Wide A peak
2) Area of A peak < 80%
3) Peak area greater than expected
4) Peak after A2
5) A1c > 10%
6) HbF or variant present
7) Total sample area too small/big
8) A2 is not within normal range