


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2022, Rack A, Plate 1, Well B12, 171542
 [896790D3207FD19F] Dec 19, 2025 10:52:24 Pressure = 75 bar (75 to 77)

FA

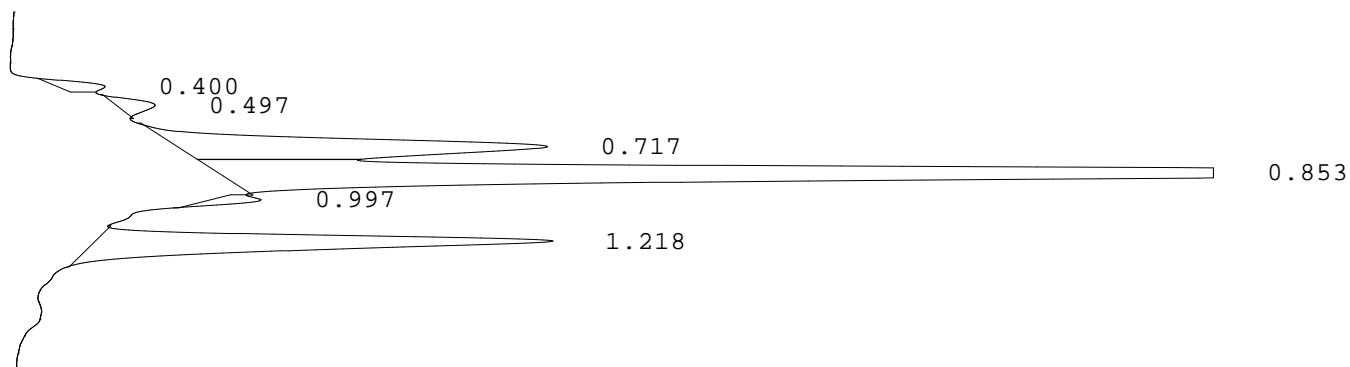

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.47	1.3%	13358	
2	0.497	F 0.59	1.5%	15257	
3	0.717	F 0.84	18.0%	188219	
4	0.853	F 1.01	59.2%	619768	Consistent with F
5	0.997	F 1.17	1.4%	14256	
6	1.218	A 1.01	18.8%	196668	A peak
Total Area:				1047526	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range