


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2140, Rack A, Plate 1, Well D02, 496419
[CD760E2E64B60E48] May 06, 2026 12:44:33 Pressure = 64 bar (63 to 66)

FA

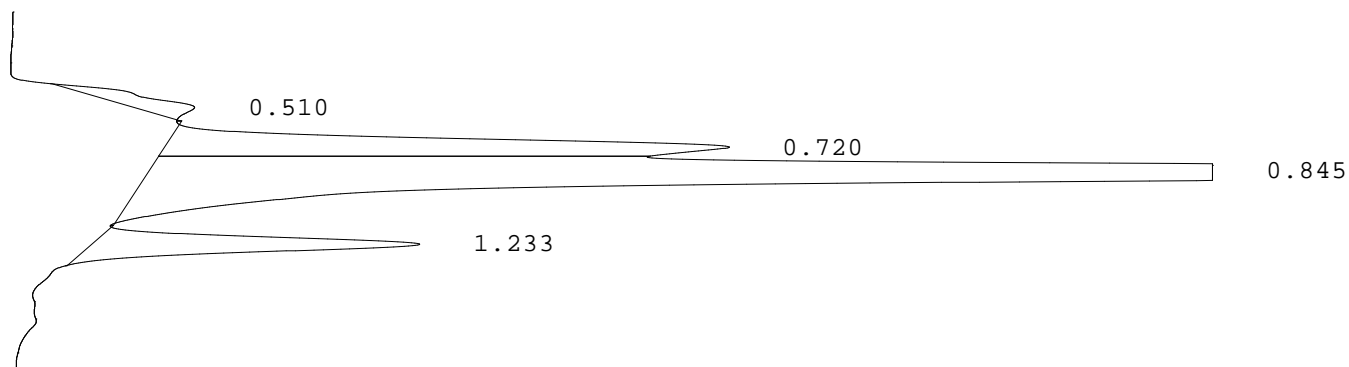

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.510	F 0.60	2.4%	42812	
2	0.720	F 0.84	16.3%	285979	Acetylated F peak
3	0.845	F 0.99	72.6%	1270321	Consistent with F
4	1.233	A 1.01	8.6%	150247	A peak
Total Area: 1749359					

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range