


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2204, Rack A, Plate 1, Well D12, 500858
[9D69D8E96F3DBB35] Jul 23, 2026 11:48:07 Pressure = 93 bar (93 to 95)

FA

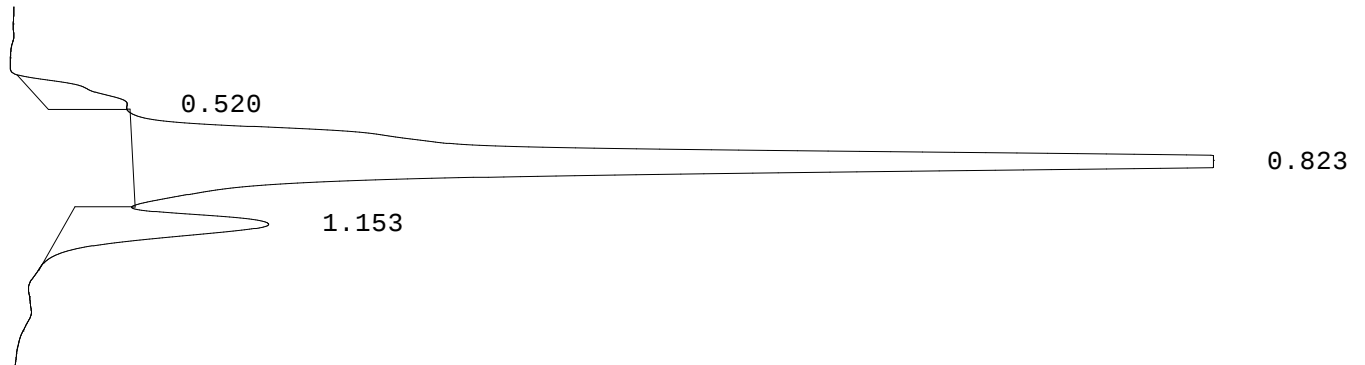

PEAK	RT	REL	RT	% CONC	AREA	COMMENT
1	0.520	F	0.63	4.7%	57082	
2	0.823	F	0.99	83.0%	1019051	Consistent with F
3	1.153	A	0.99	12.3%	151013	A peak
Total Area: 1227146						

Codes: 1) Wide A peak
2) Area of A peak < 80%
3) Peak area greater than expected
4) Peak after A2
5) A1c > 10%
6) HbF or variant present
7) Total sample area too small/big
8) A2 is not within normal range