


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2046, Rack A, Plate 1, Well B08, 488976
 [CD679D396CC0A6EA] Jan 16, 2026 10:40:28 Pressure = 85 bar (84 to 87)

FA

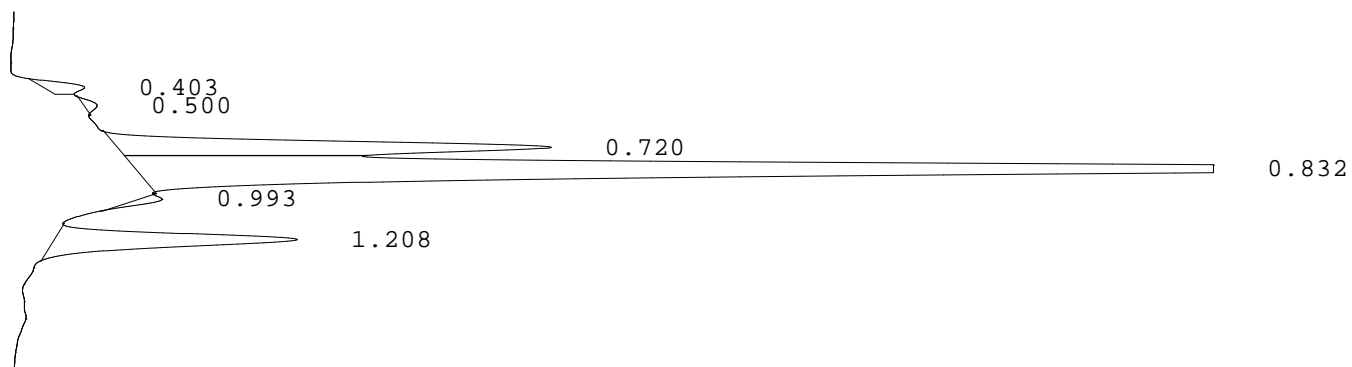

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.48	1.4%	12454	
2	0.500	F 0.60	0.5%	4618	
3	0.720	F 0.86	18.4%	162558	Acetylated F peak
4	0.832	F 0.99	67.5%	595182	Consistent with F
5	0.993	F 1.18	0.9%	8016	
6	1.208	A 1.02	11.2%	99171	A peak
Total Area:				881999	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range