


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2179, Rack A, Plate 1, Well E11, 485914
[8828AEC17FCF3117] Jun 18, 2026 14:35:14 Pressure = 70 bar (70 to 72)

FA

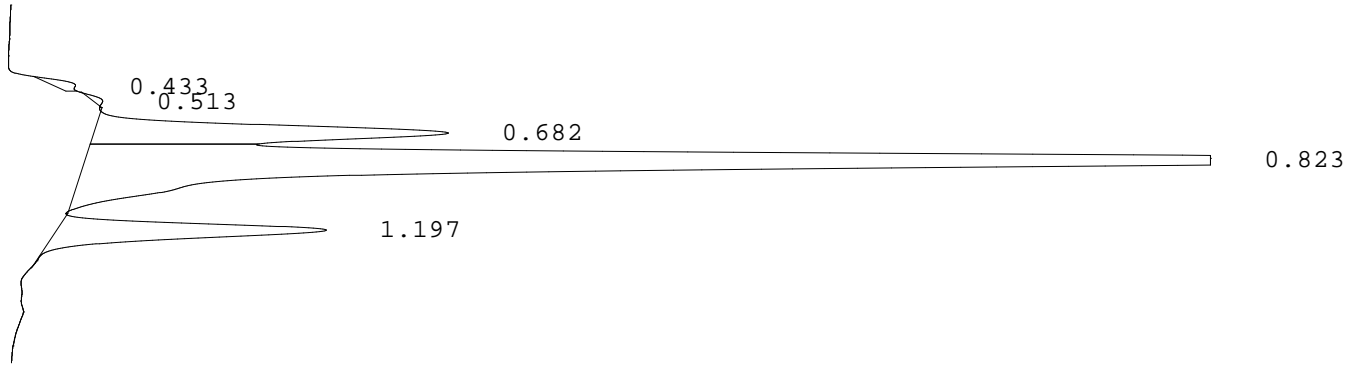

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.433	F 0.52	0.7%	7240	
2	0.513	F 0.61	0.3%	3275	
3	0.682	F 0.81	15.6%	168006	Acetylated F peak
4	0.823	F 0.98	72.2%	779302	Consistent with F
5	1.197	A 1.01	11.3%	121570	A peak
Total Area:				1079393	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range