


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2018, Rack A, Plate 1, Well G02, 486852  
 [8D23D1A150F5DB17] Dec 15, 2025 12:04:02 Pressure = 73 bar (72 to 74)

FA

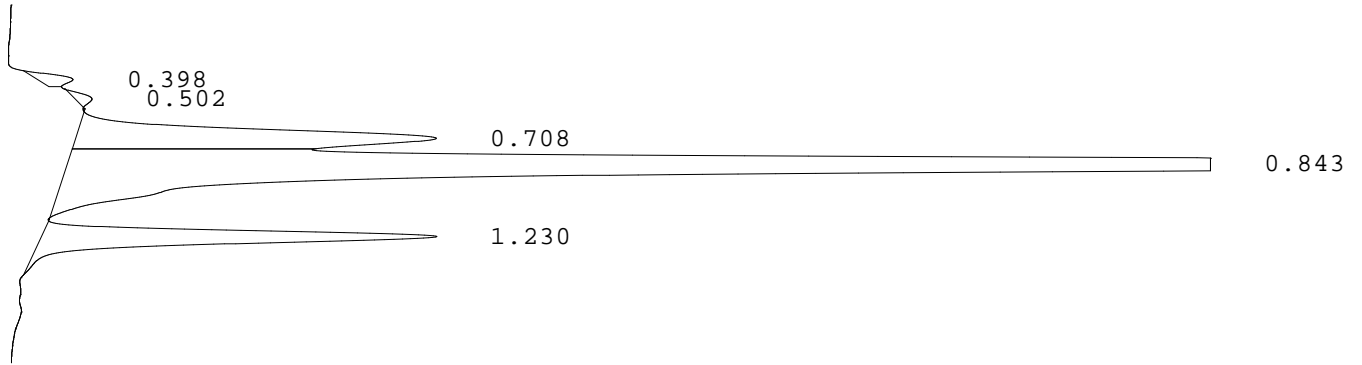

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.46	0.8%	10605	
2	0.502	F 0.59	0.4%	5867	
3	0.708	F 0.83	13.8%	192874	Acetylated F peak
4	0.843	F 0.98	73.7%	1031739	Consistent with F
5	1.230	A 1.01	11.3%	158508	A peak
Total Area:				1399593	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range