


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1359, Rack A, Plate 1, Well C01, 27481
[CCD8A1127450E0EA] Apr 03, 2024 10:21:32 Pressure = 61 bar (61 to 61)

FA

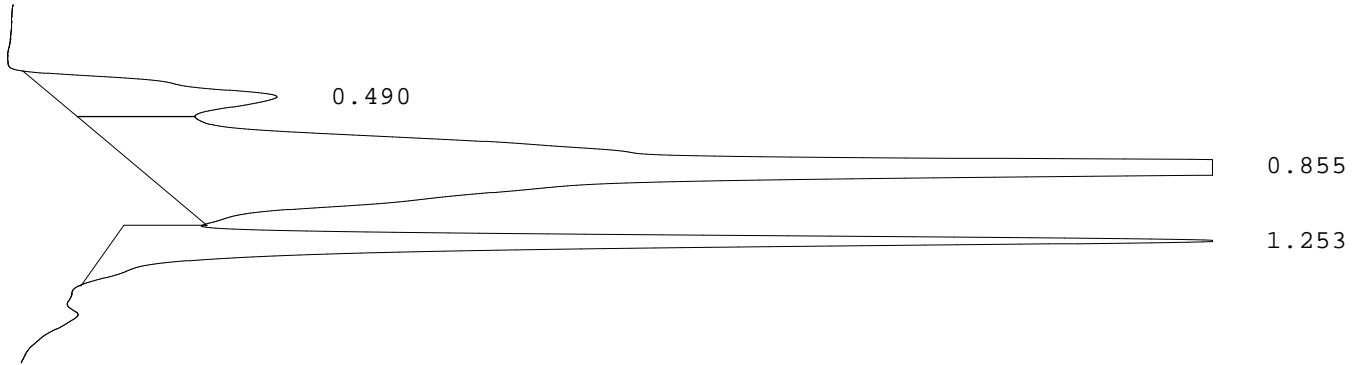

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.490	F 0.57	8.5%	187455	
2	0.855	F 0.99	69.3%	1526801	Consistent with F
3	1.253	A 1.00	22.2%	487797	A peak - REVIEW
Total Area:				2202053	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range