


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2029, Rack A, Plate 1, Well F01, 171696
[997382B8BA080EC2] Dec 29, 2025 12:57:30 Pressure = 74 bar (74 to 76)

FA

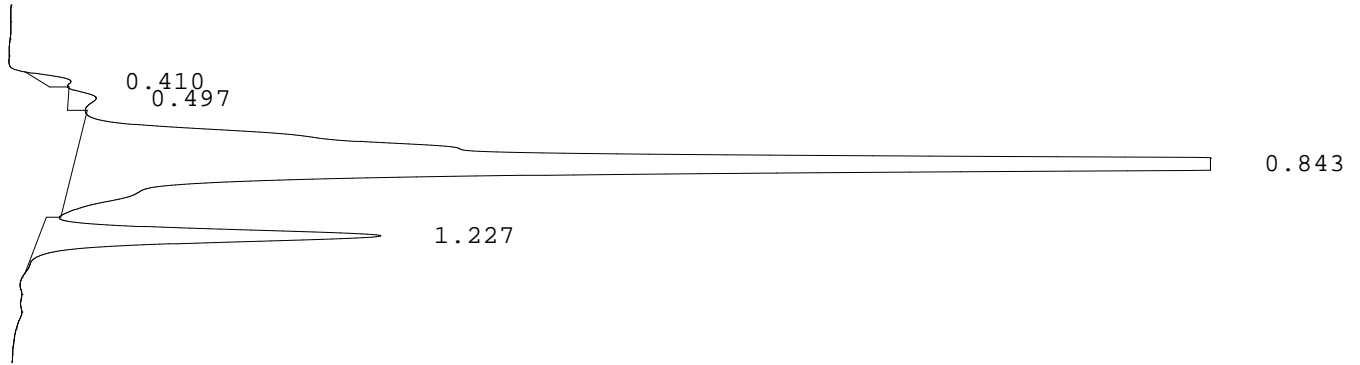

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.48	0.7%	9407	
2	0.497	F 0.58	1.0%	13019	
3	0.843	F 0.98	87.5%	1169587	Consistent with F
4	1.227	A 1.01	10.8%	144949	A peak
Total Area:				1336962	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range