


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1957, Rack A, Plate 1, Well A08, 170725
 [CD241A7F99498660] Oct 24, 2025 09:48:07 Pressure = 69 bar (69 to 71)

FA

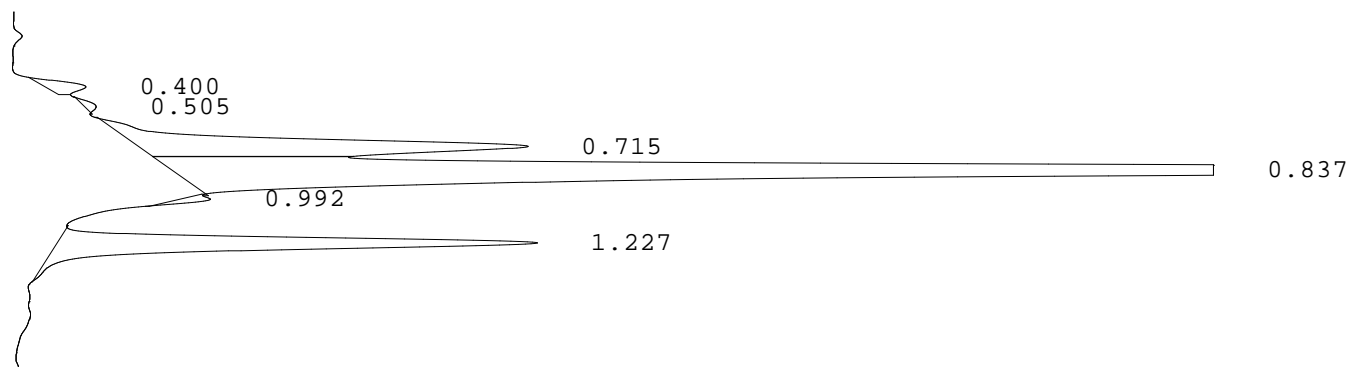

| PEAK | RT | REL RT | % CONC | AREA | COMMENT |
|-------------|-------|--------|--------|---------|-------------------|
| 1 | 0.400 | F 0.47 | 1.1% | 12813 | |
| 2 | 0.505 | F 0.59 | 0.4% | 3958 | |
| 3 | 0.715 | F 0.84 | 15.8% | 177577 | Acetylated F peak |
| 4 | 0.837 | F 0.98 | 66.1% | 743217 | Consistent with F |
| 5 | 0.992 | F 1.16 | 0.7% | 7870 | |
| 6 | 1.227 | A 1.00 | 15.9% | 178781 | A peak |
| Total Area: | | | | 1124216 | |

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range