


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well C01, 484358
 [DD2285F407202CCA] Dec 15, 2025 10:20:56 Pressure = 74 bar (74 to 77)

FA

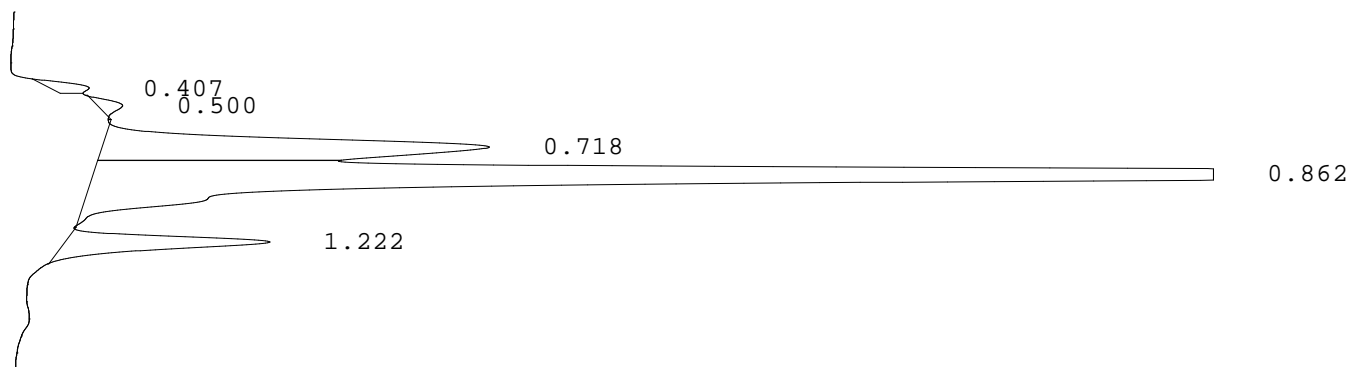

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	1.0%	11487	
2	0.500	F 0.59	0.8%	9645	
3	0.718	F 0.85	18.6%	221232	Acetylated F peak
4	0.862	F 1.01	72.8%	866341	Consistent with F
5	1.222	A 1.01	6.8%	80767	A peak
Total Area:				1189472	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range