


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2025, Rack A, Plate 1, Well G11, 486826
 [DC268578B32AA4E8] Dec 23, 2025 13:52:45 Pressure = 75 bar (74 to 77)

FA

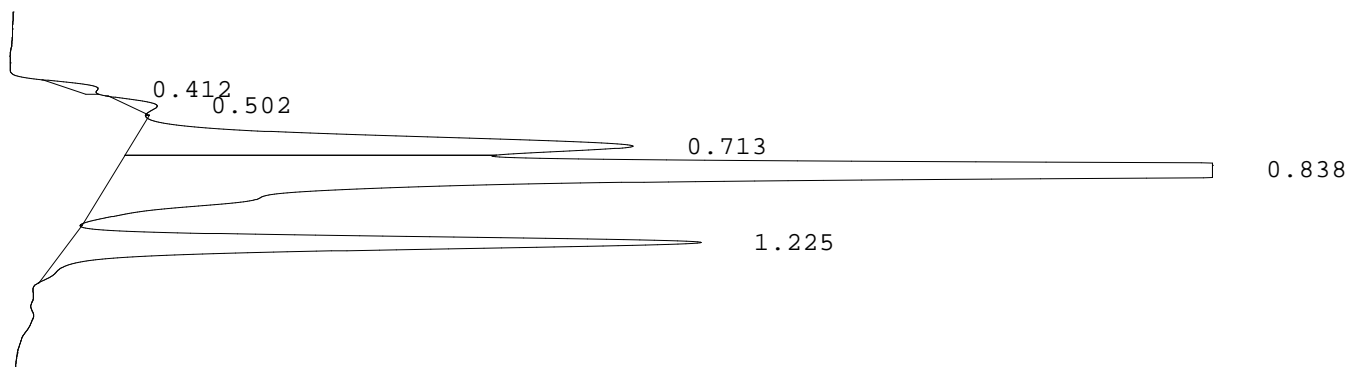

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.412	F 0.47	0.5%	9098	
2	0.502	F 0.58	0.6%	10092	
3	0.713	F 0.82	15.5%	273446	Acetylated F peak
4	0.838	F 0.97	68.3%	1204374	Consistent with F
5	1.225	A 1.01	15.0%	265123	A peak
Total Area:				1762133	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range