


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well D03, 484362
 [DC22D1F407A22440] Dec 15, 2025 10:51:15 Pressure = 74 bar (73 to 76)

FA

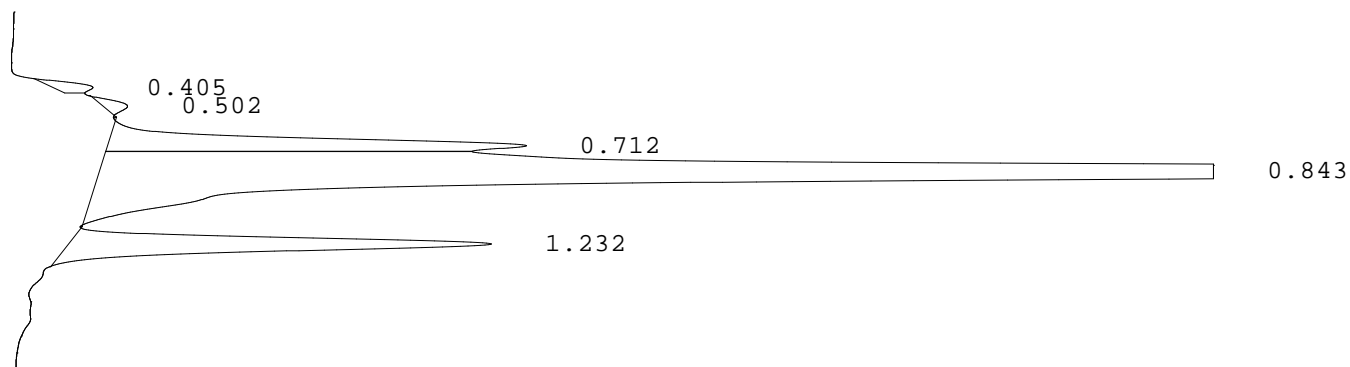

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	0.7%	11616	
2	0.502	F 0.59	0.6%	9219	
3	0.712	F 0.83	10.1%	162731	Acetylated F peak
4	0.843	F 0.98	77.9%	1258903	Consistent with F
5	1.232	A 1.01	10.8%	174329	A peak
Total Area:				1616798	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range