


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2068, Rack A, Plate 1, Well F12, 492221
 [9D33647B310E0EE2] Feb 10, 2026 12:51:10 Pressure = 94 bar (94 to 97)

FA

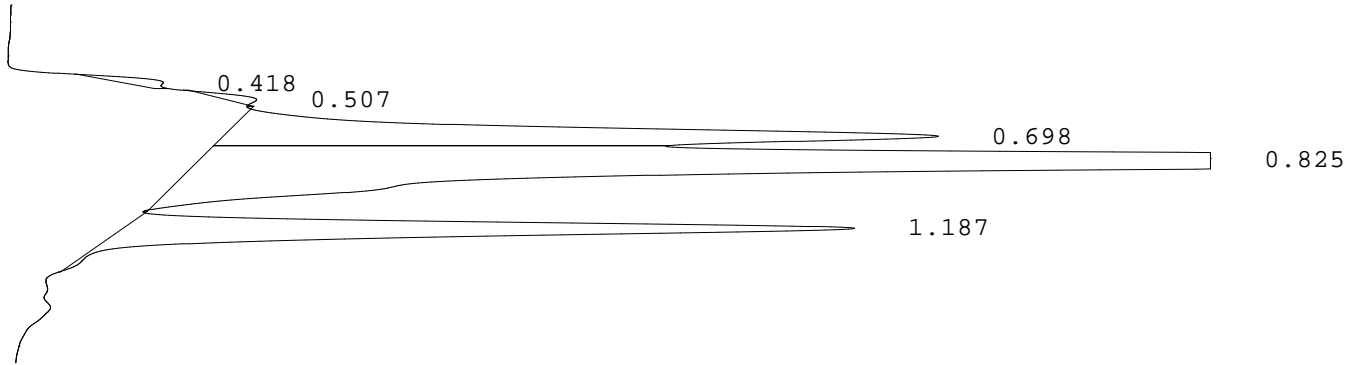

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.418	F 0.50	0.6%	12998	
2	0.507	F 0.60	0.5%	10483	
3	0.698	F 0.83	17.5%	357451	Acetylated F peak
4	0.825	F 0.98	65.7%	1339858	Consistent with F
5	1.187	A 1.00	15.6%	319046	A peak
Total Area:				2039836	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range