


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2113, Rack A, Plate 1, Well B05, 498239  
[997256830001F3BD] Apr 07, 2026 11:42:21 Pressure = 59 bar (59 to 61)

FA

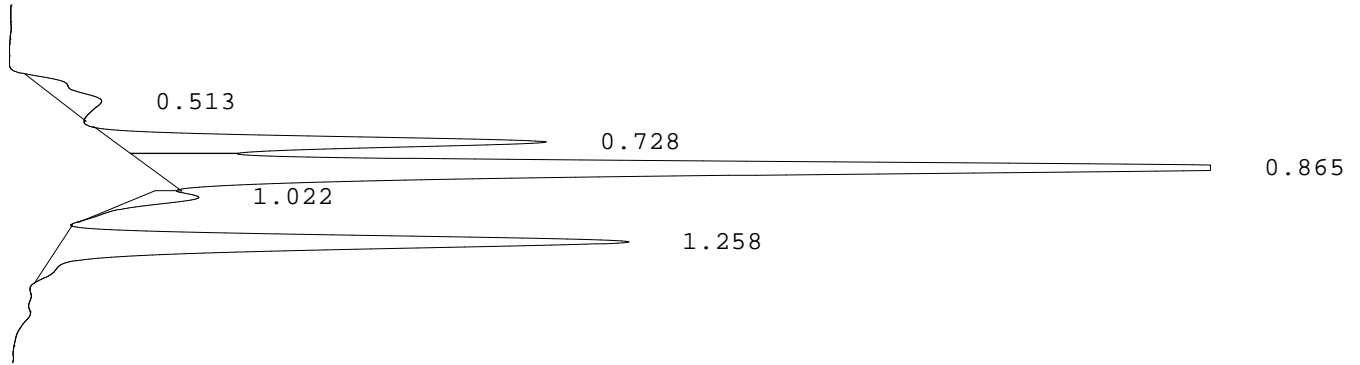

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.513	F 0.59	3.4%	33457	
2	0.728	F 0.84	16.3%	158363	
3	0.865	F 1.00	51.9%	503455	Consistent with F
4	1.022	F 1.18	2.5%	24593	
5	1.258	A 1.01	25.8%	250343	A peak - REVIEW
Total Area:				970211	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range