


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1988, Rack A, Plate 1, Well A12, 171109
 [CD67A9E08FBA8C40] Nov 21, 2025 11:00:19 Pressure = 70 bar (70 to 72)

FA

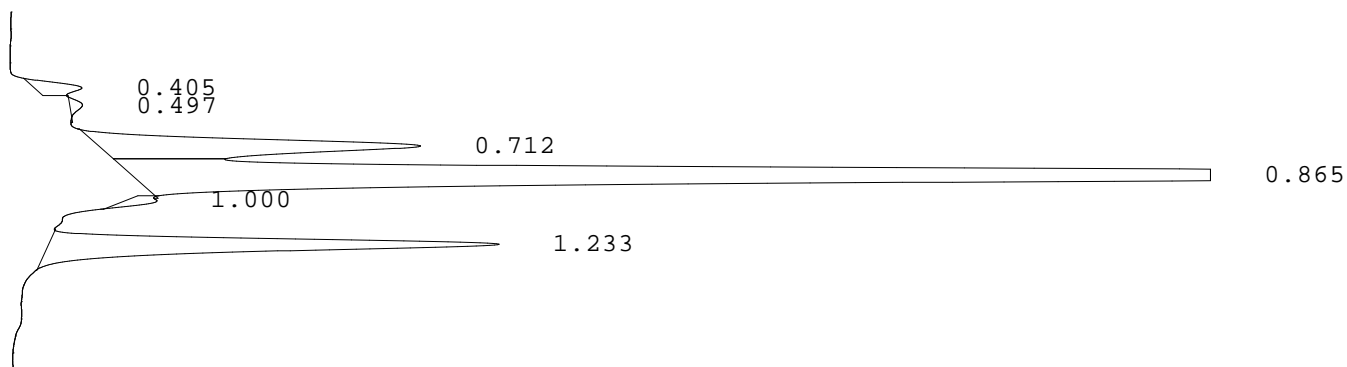

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	1.4%	15156	
2	0.497	F 0.58	0.4%	4850	
3	0.712	F 0.83	12.9%	142637	Acetylated F peak
4	0.865	F 1.01	68.8%	758221	Consistent with F
5	1.000	F 1.17	0.9%	9737	
6	1.233	A 1.01	15.6%	171410	A peak
Total Area:				1102011	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range