


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2022, Rack A, Plate 1, Well D09, 484373  
 [9826D18675A0066A] Dec 19, 2025 11:36:52 Pressure = 76 bar (75 to 78)

FA

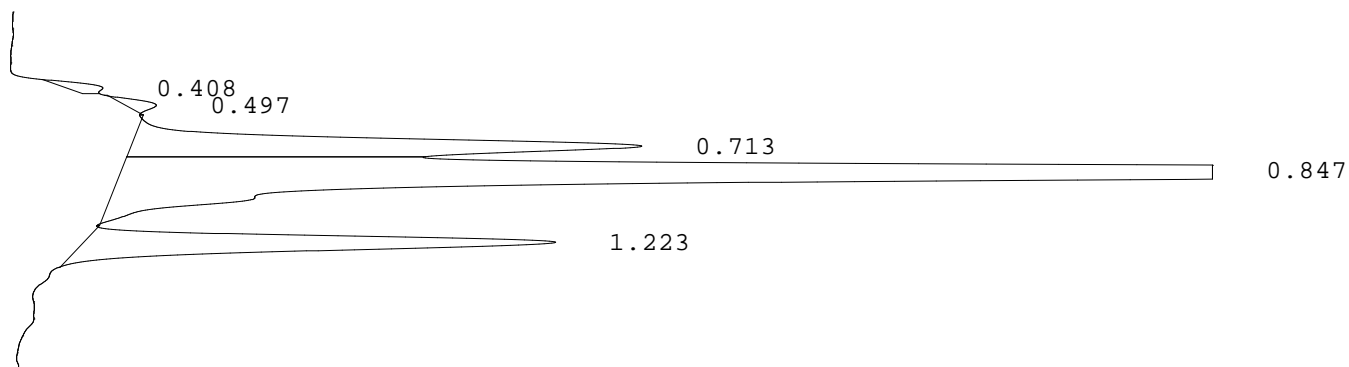

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.408	F 0.48	0.7%	10714	
2	0.497	F 0.58	0.7%	10630	
3	0.713	F 0.83	15.3%	247632	Acetylated F peak
4	0.847	F 0.99	70.3%	1134218	Consistent with F
5	1.223	A 1.01	13.0%	210573	A peak
Total Area:				1613767	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range