


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2054, Rack A, Plate 1, Well F05, 483331
[9D23DFDF97C20EEA] Jan 26, 2026 12:53:16 Pressure = 87 bar (86 to 89)

FA

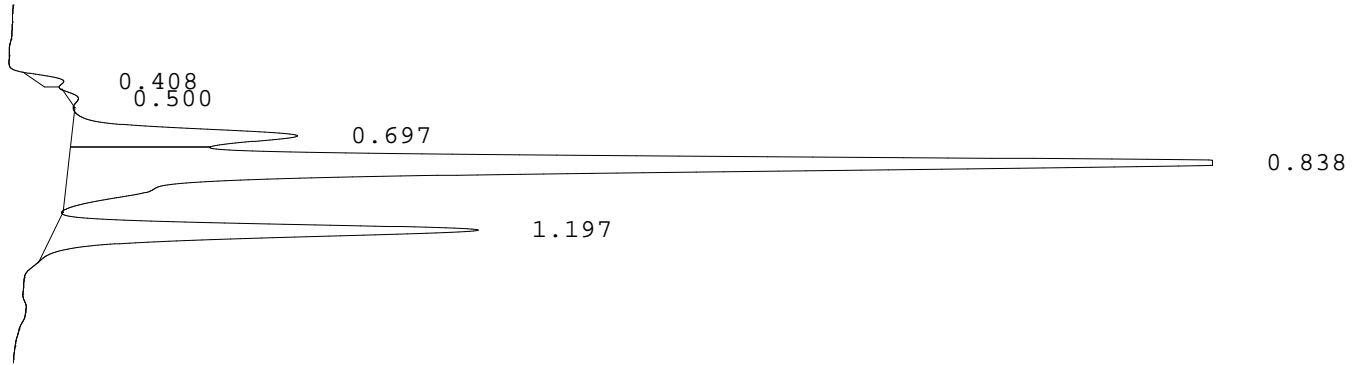

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.408	F 0.48	0.9%	8201	
2	0.500	F 0.58	0.4%	3395	
3	0.697	F 0.81	11.7%	111152	Acetylated F peak
4	0.838	F 0.98	68.0%	645852	Consistent with F
5	1.197	A 1.01	19.1%	181191	A peak
Total Area:				949791	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range