


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1801, Rack A, Plate 1, Well B02, 455885
[DC31F847A3B2D91F] May 21, 2025 10:17:36 Pressure = 60 bar (59 to 61)

FA

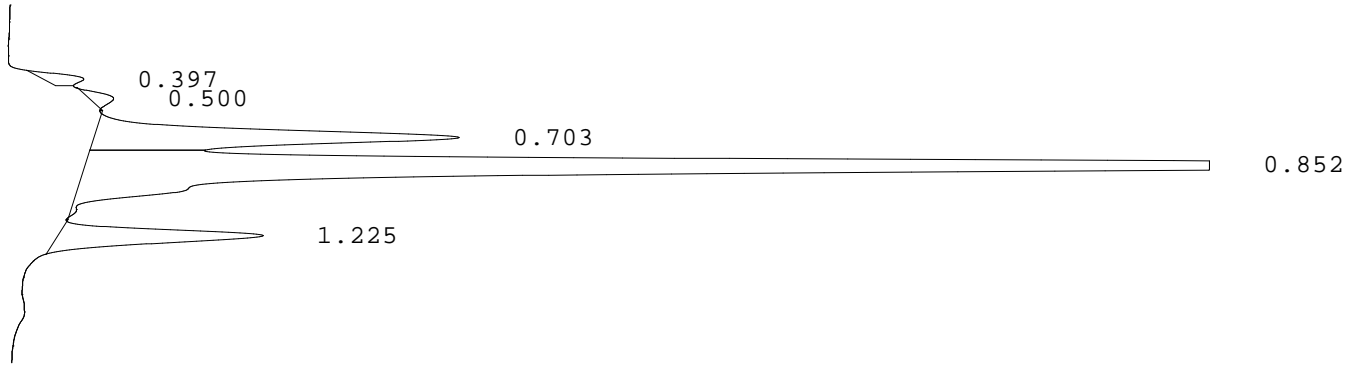

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.397	F 0.47	1.2%	12139	
2	0.500	F 0.59	1.0%	9457	
3	0.703	F 0.83	17.4%	169878	Acetylated F peak
4	0.852	F 1.01	71.9%	703311	Consistent with F
5	1.225	A 1.01	8.5%	83426	A peak
Total Area:				978211	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range