


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1977, Rack A, Plate 1, Well F09, 478846
[CD22B7CE622579B5] Nov 14, 2025 12:31:11 Pressure = 68 bar (67 to 70)

FA

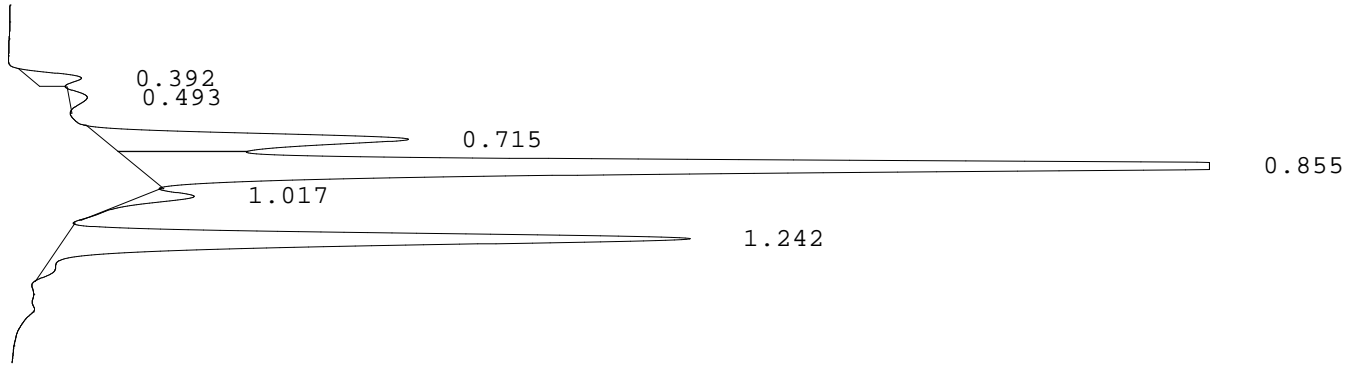

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.392	F 0.45	1.8%	17153	
2	0.493	F 0.57	0.8%	7300	
3	0.715	F 0.83	13.3%	127688	Acetylated F peak
4	0.855	F 0.99	56.1%	536816	Consistent with F
5	1.017	F 1.18	2.0%	18835	
6	1.242	A 1.01	26.1%	249828	A peak - REVIEW
Total Area:				957620	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range