


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2130, Rack A, Plate 1, Well F11, 502218
 [C966097F919E04E0] Apr 24, 2026 13:36:47 Pressure = 62 bar (61 to 63)

FA

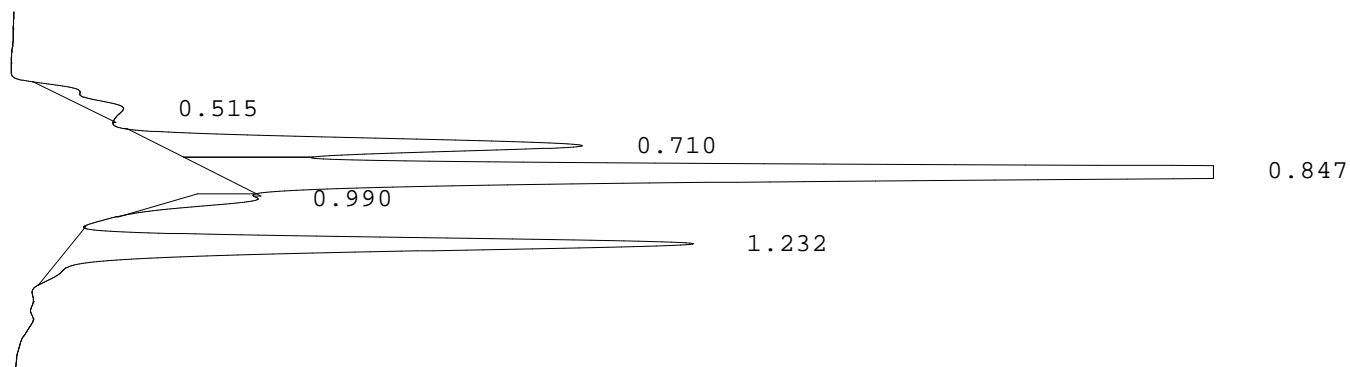

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.515	F 0.60	2.1%	27026	
2	0.710	F 0.82	14.6%	187116	Acetylated F peak
3	0.847	F 0.98	59.6%	765745	Consistent with F
4	0.990	F 1.15	2.4%	30327	
5	1.232	A 1.00	21.4%	274363	A peak - REVIEW
Total Area:				1284577	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range