


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2061, Rack A, Plate 1, Well C09, 489182
 [DD73DB10A960244A] Jan 30, 2026 11:08:16 Pressure = 90 bar (90 to 92)

FA

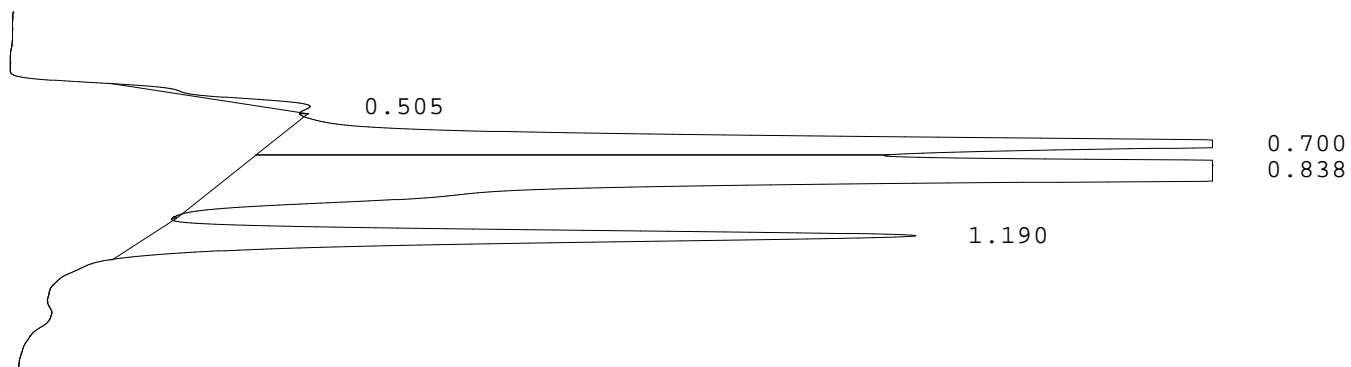

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.505	F 0.60	1.0%	28215	
2	0.700	F 0.83	19.1%	542894	Acetylated F peak
3	0.838	F 1.00	68.9%	1962314	Consistent with F
4	1.190	A 1.00	11.1%	316359	A peak
Total Area:				2849782	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range