


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2185, Rack A, Plate 1, Well B09, 493544
[C93DBF03236FB33D] Jun 25, 2026 12:27:01 Pressure = 72 bar (72 to 74)

FA

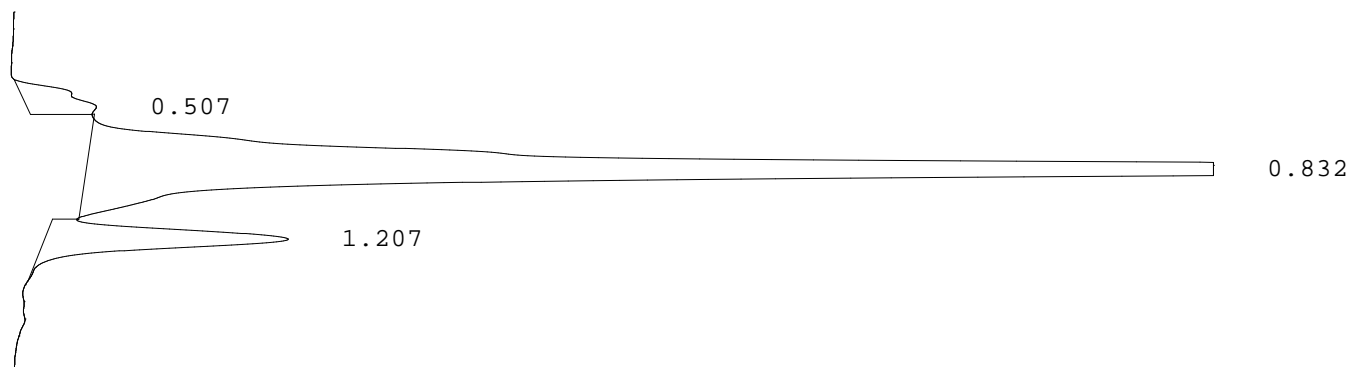

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.507	F 0.61	3.5%	47105	
2	0.832	F 0.99	85.8%	1138932	Consistent with F
3	1.207	A 1.02	10.6%	140870	A peak

Total Area: 1326907

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range