


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2182, Rack A, Plate 1, Well C12, 486014
[D829FA2DC412C64A] Jun 23, 2026 11:21:52 Pressure = 72 bar (72 to 75)

FA

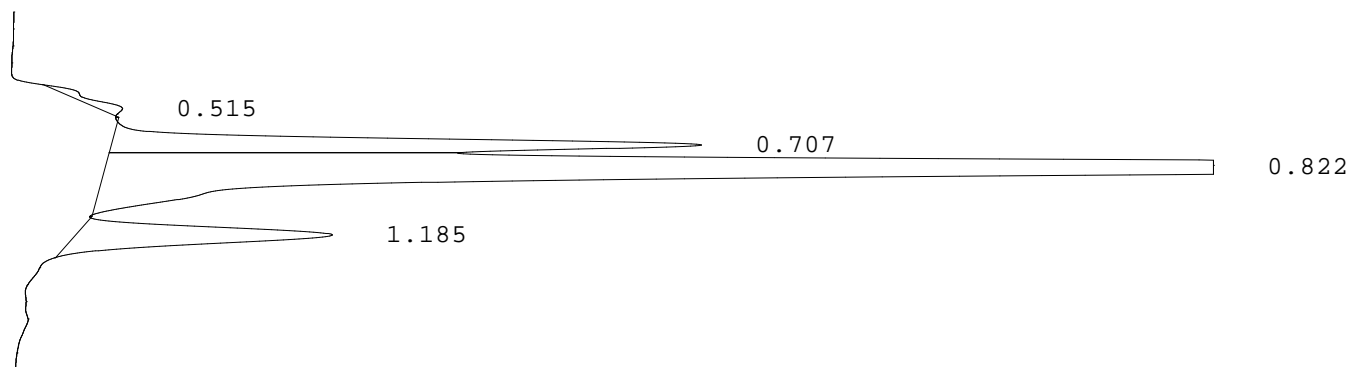

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.515	F 0.61	1.1%	15100	
2	0.707	F 0.83	15.8%	222584	Acetylated F peak
3	0.822	F 0.97	73.8%	1037079	Consistent with F
4	1.185	A 1.01	9.3%	130244	A peak
Total Area:				1405007	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range