


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2188, Rack A, Plate 1, Well B01, 493024
[882DC1D300FD33B7] Jul 01, 2026 11:16:46 Pressure = 79 bar (79 to 81)

FA

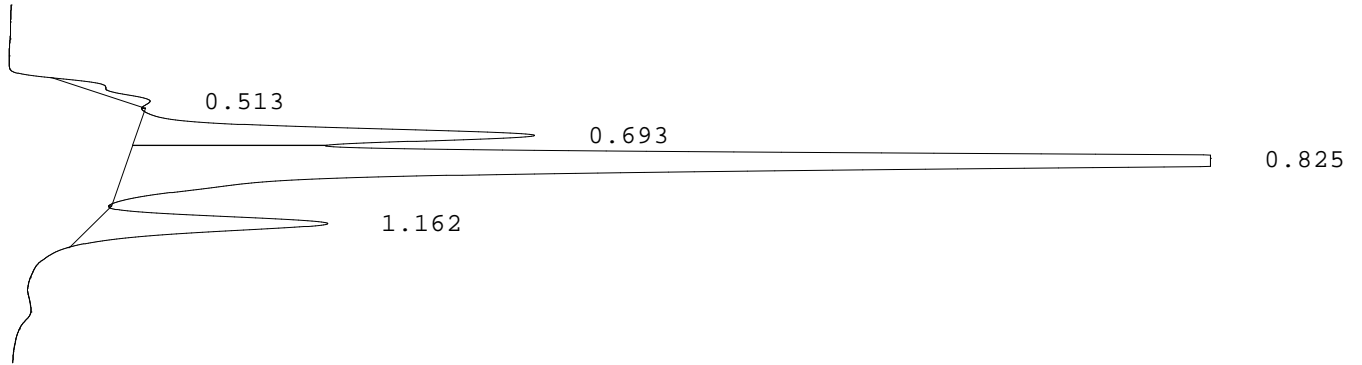

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.513	F 0.61	1.7%	19125	
2	0.693	F 0.83	15.9%	181539	Acetylated F peak
3	0.825	F 0.98	72.4%	825147	Consistent with F
4	1.162	A 1.00	10.0%	113622	A peak
Total Area: 1139433					

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range