


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2080, Rack A, Plate 1, Well D01, 492111
[CD332312FC2E0EE8] Feb 24, 2026 11:38:37 Pressure = 57 bar (56 to 58)

FA

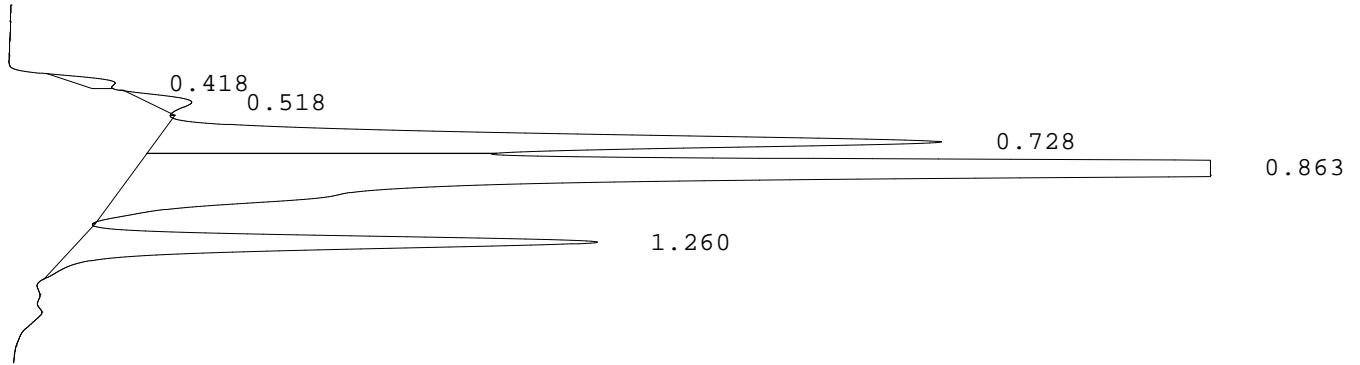

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.418	F 0.48	0.6%	12764	
2	0.518	F 0.59	0.9%	18977	
3	0.728	F 0.83	19.0%	383281	Acetylated F peak
4	0.863	F 0.98	68.4%	1381665	Consistent with F
5	1.260	A 1.01	11.0%	223180	A peak
Total Area:				2019867	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range