


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1974, Rack A, Plate 1, Well D06, 482298
[DD32B2EE65508CE0] Nov 11, 2025 12:34:23 Pressure = 66 bar (66 to 68)

FA

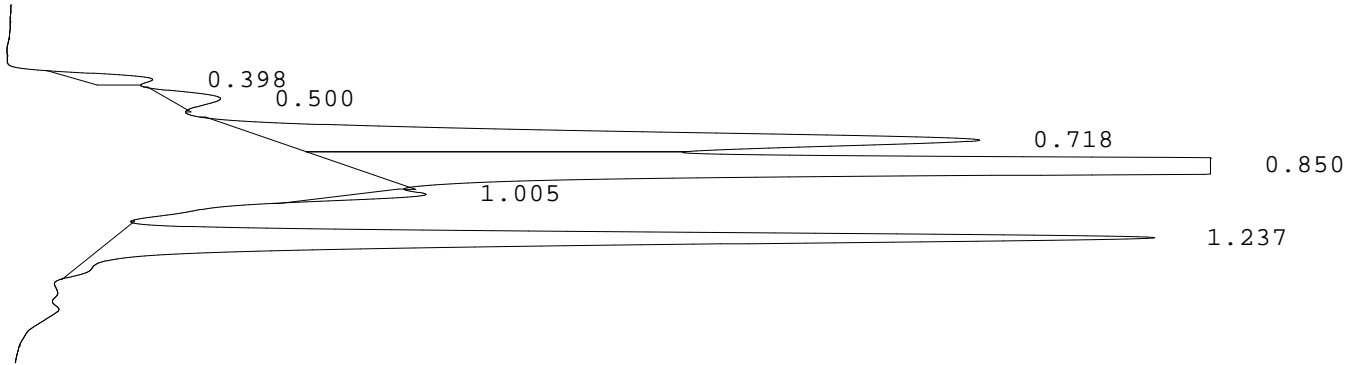

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.46	1.1%	22326	
2	0.500	F 0.58	1.1%	21684	
3	0.718	F 0.83	18.6%	375711	
4	0.850	F 0.98	57.2%	1154846	Consistent with F
5	1.005	F 1.16	1.1%	21952	
6	1.237	A 1.00	20.9%	422502	A peak - REVIEW

Total Area: 2019021

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range