


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2149, Rack A, Plate 1, Well C11, 501895  
[CD3DA407A187913F] May 20, 2026 13:17:24 Pressure = 65 bar (65 to 66)

FA

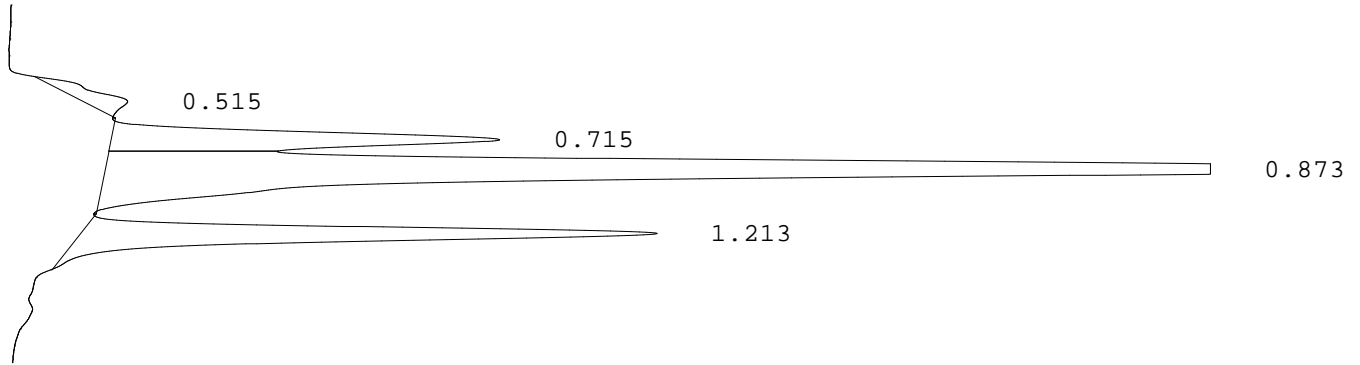

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.515	F 0.60	2.5%	31718	
2	0.715	F 0.83	14.3%	180283	Acetylated F peak
3	0.873	F 1.02	63.0%	792515	Consistent with F
4	1.213	A 1.00	20.2%	254065	A peak - REVIEW
Total Area: 1258581					

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range