


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1957, Rack A, Plate 1, Well D01, 170744
 [CD715E7F99E1ACE8] Oct 24, 2025 10:48:45 Pressure = 68 bar (68 to 70)

FA

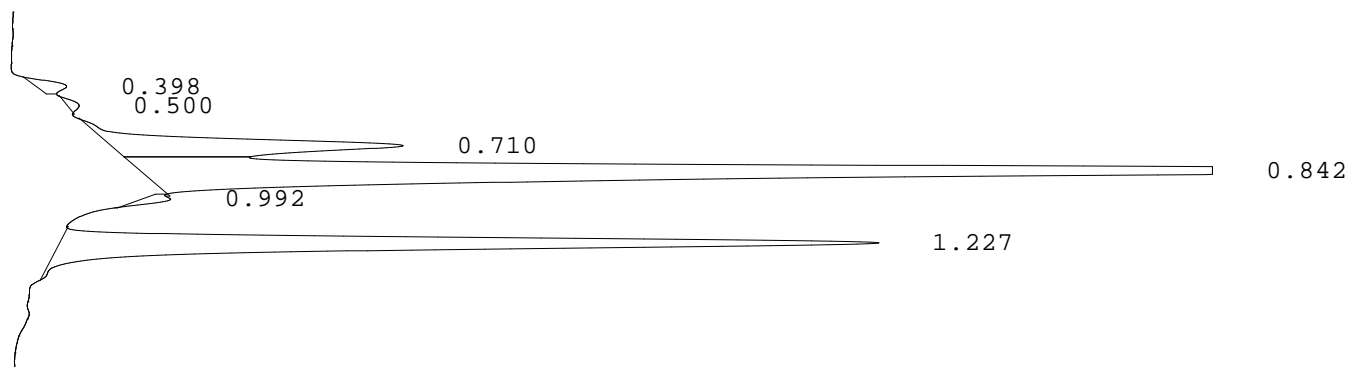

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.398	F 0.46	0.9%	9663	
2	0.500	F 0.58	0.4%	4014	
3	0.710	F 0.83	12.2%	125235	Acetylated F peak
4	0.842	F 0.98	56.5%	578937	Consistent with F
5	0.992	F 1.16	0.8%	8560	
6	1.227	A 1.00	29.1%	298448	A peak - REVIEW
Total Area:				1024857	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range