


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well D07, 486536
 [9962C0F4050A2CCA] Dec 15, 2025 10:59:20 Pressure = 73 bar (72 to 75)

FA

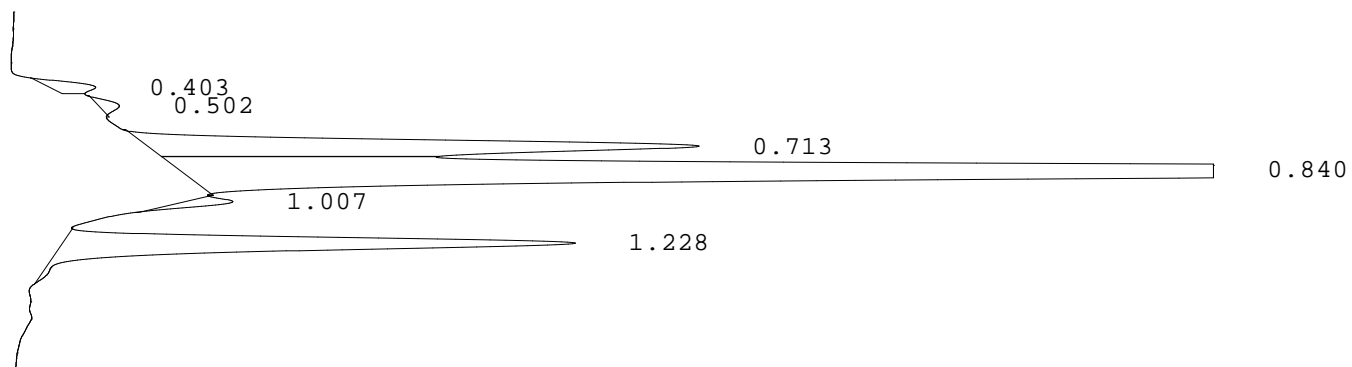

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.403	F 0.47	1.0%	14119	
2	0.502	F 0.59	0.5%	7644	
3	0.713	F 0.83	16.3%	226570	Acetylated F peak
4	0.840	F 0.98	66.5%	927206	Consistent with F
5	1.007	F 1.18	1.0%	14586	
6	1.228	A 1.01	14.6%	204096	A peak
Total Area:				1394221	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range