


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2022, Rack A, Plate 1, Well H02, 171593  
[DC76D59788555B9D] Dec 19, 2025 13:01:45 Pressure = 73 bar (73 to 75)

FA

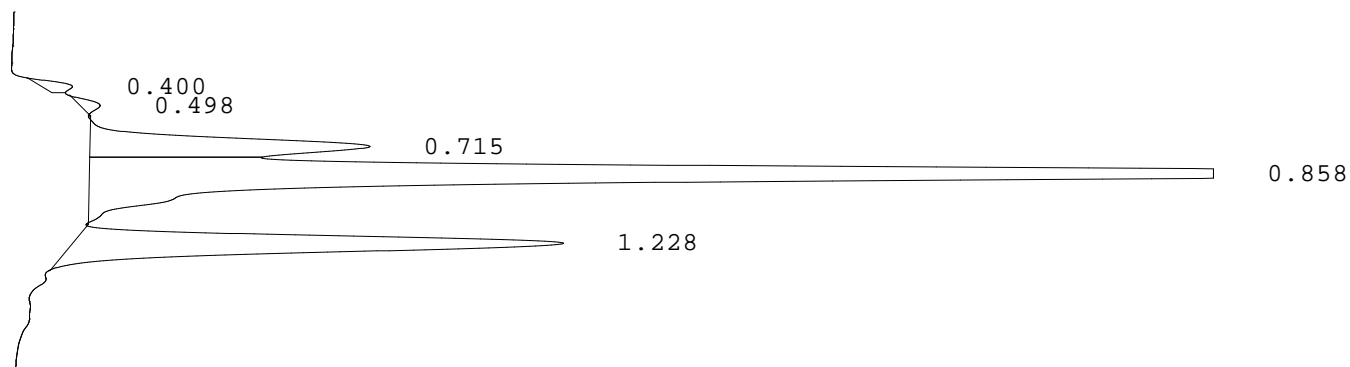

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.47	0.8%	8944	
2	0.498	F 0.58	0.6%	7098	
3	0.715	F 0.83	12.5%	142989	Acetylated F peak
4	0.858	F 1.00	64.7%	740864	Consistent with F
5	1.228	A 1.01	21.4%	245125	A peak - REVIEW

Total Area: 1145020

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range