


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2029, Rack A, Plate 1, Well C11, 490128
[8D23D2FDC57F51B5] Dec 29, 2025 12:02:55 Pressure = 75 bar (74 to 77)

FA

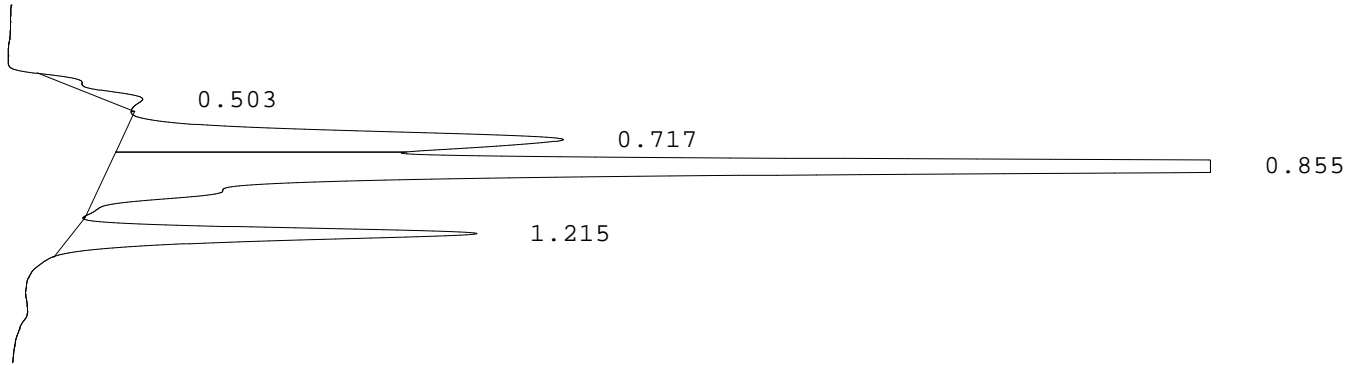

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.503	F 0.59	1.8%	24842	
2	0.717	F 0.84	18.4%	254701	Acetylated F peak
3	0.855	F 1.00	68.1%	943492	Consistent with F
4	1.215	A 1.01	11.7%	162754	A peak
Total Area:				1385789	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range