


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 1960, Rack A, Plate 1, Well A10, 478819  
 [CD33E4F0AD8D59B7] Oct 28, 2025 09:54:22 Pressure = 68 bar (67 to 70)

FA

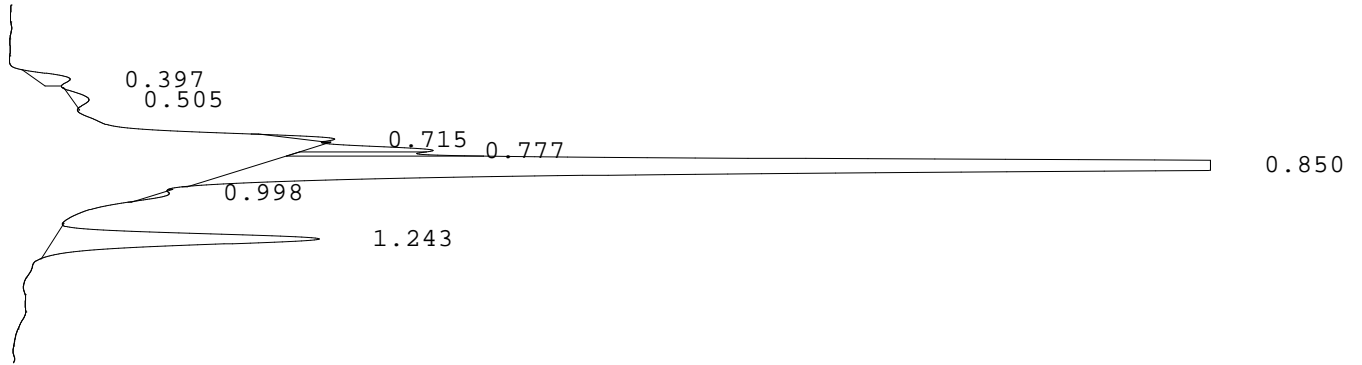

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.397	F 0.46	1.4%	10942	
2	0.505	F 0.59	0.8%	6367	
3	0.715	F 0.83	0.9%	6978	
4	0.777	F 0.91	4.9%	37662	
5	0.850	F 0.99	78.7%	600609	Consistent with F
6	0.998	F 1.17	0.5%	3775	
7	1.243	A 1.01	12.7%	96786	A peak
Total Area:				763119	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range