


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2130, Rack A, Plate 1, Well H01, 502909  
[CD62197F91B6A648] Apr 24, 2026 14:05:05 Pressure = 61 bar (61 to 63)

FA

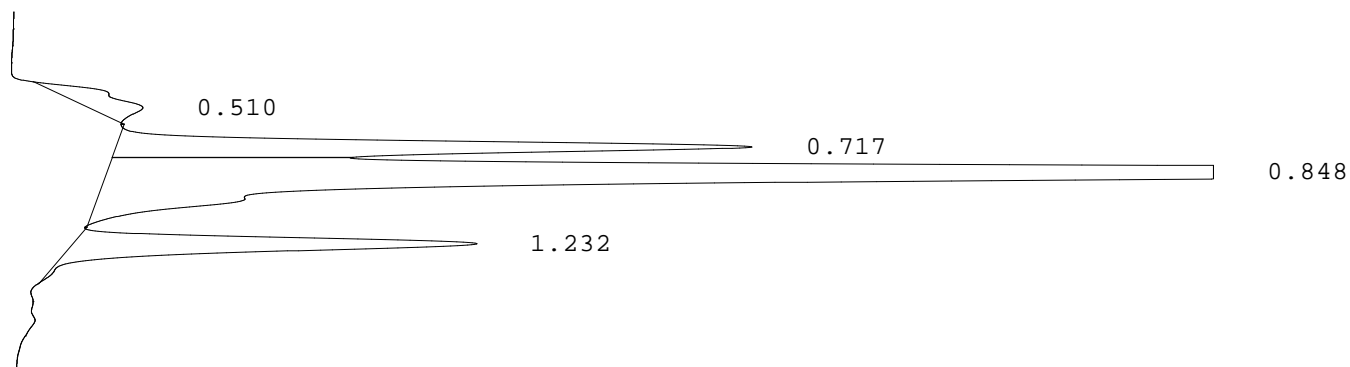

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.510	F 0.59	3.0%	43954	
2	0.717	F 0.83	16.7%	244370	Acetylated F peak
3	0.848	F 0.98	68.6%	1006381	Consistent with F
4	1.232	A 1.00	11.8%	172826	A peak
Total Area: 1467531					

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range