


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1801, Rack A, Plate 1, Well B11, 168251 FA
 [8C31FC12F447AC6A] May 21, 2025 10:35:48 Pressure = 59 bar (59 to 61)

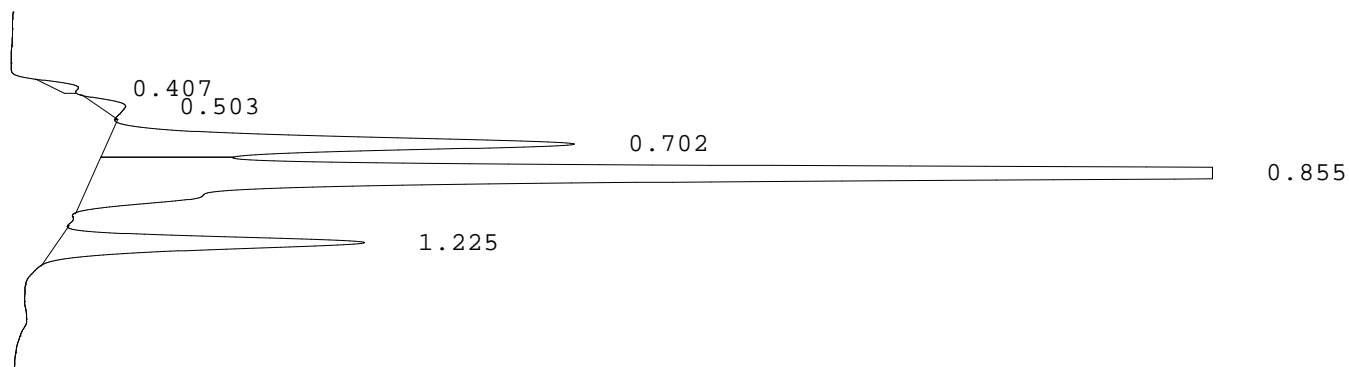

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	0.6%	7555	
2	0.503	F 0.60	1.0%	11822	
3	0.702	F 0.83	17.7%	214659	Acetylated F peak
4	0.855	F 1.01	70.5%	854260	Consistent with F
5	1.225	A 1.01	10.2%	123010	A peak
Total Area:				1211306	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range