


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 1359, Rack A, Plate 1, Well H12, 27404  
 [CDD8A456DC704AC2] Apr 03, 2024 12:51:06

Pressure = 59 bar (59 to 59)

FA

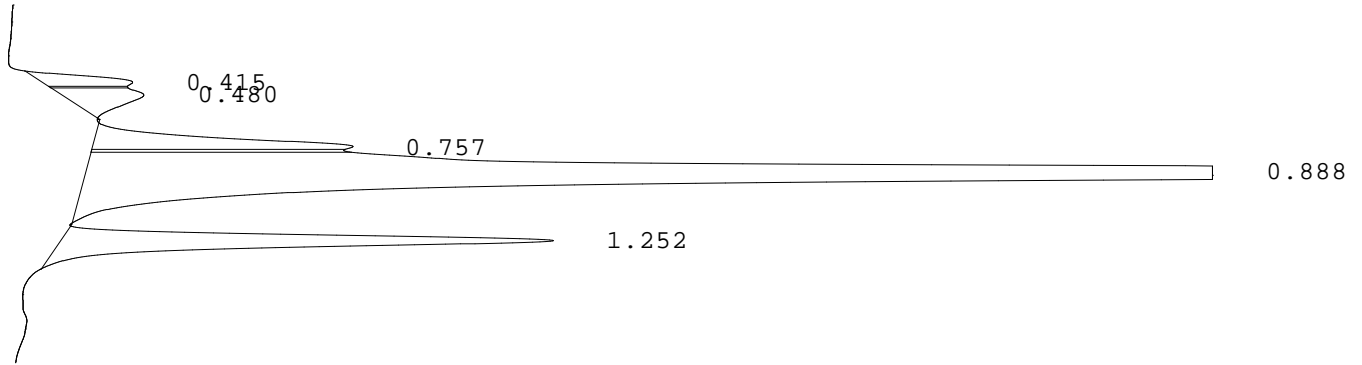

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.415	F 0.46	1.9%	30370	
2	0.480	F 0.54	2.9%	46616	
3	0.757	F 0.85	6.9%	109777	
4	0.888	F 0.99	76.5%	1220748	Consistent with F
5	1.252	A 1.00	11.8%	188142	A peak
Total Area:				1595653	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range