


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2029, Rack A, Plate 1, Well H05, 490097
[D822C6B8BAA2AE62] Dec 29, 2025 13:56:06 Pressure = 74 bar (73 to 75)

FA

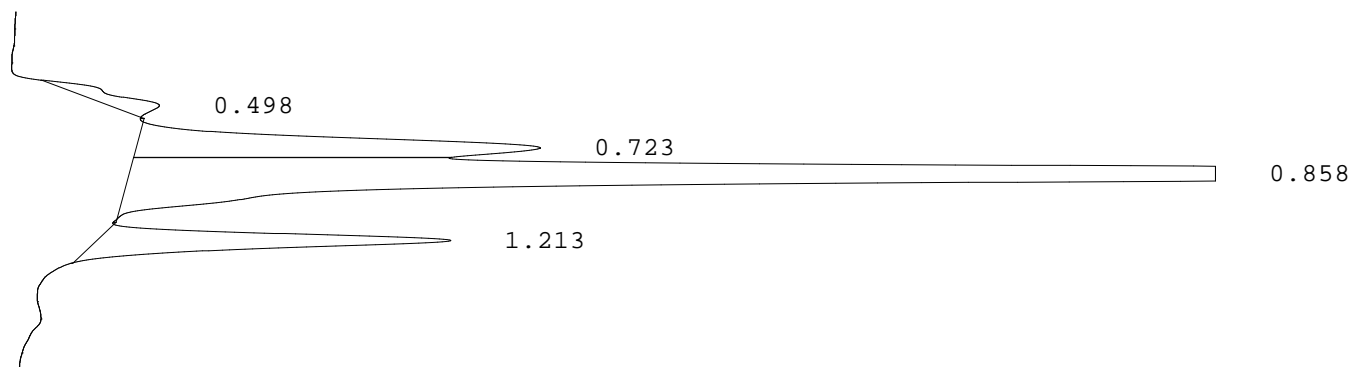

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.498	F 0.58	2.3%	34405	
2	0.723	F 0.84	15.1%	226549	Acetylated F peak
3	0.858	F 1.00	72.1%	1080242	Consistent with F
4	1.213	A 1.00	10.5%	157914	A peak
Total Area:				1499110	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range