


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1359, Rack A, Plate 1, Well G03, 27473
[DC99B0038BAF9DB7] Apr 03, 2024 12:06:38

Pressure = 59 bar (59 to 59)

FA

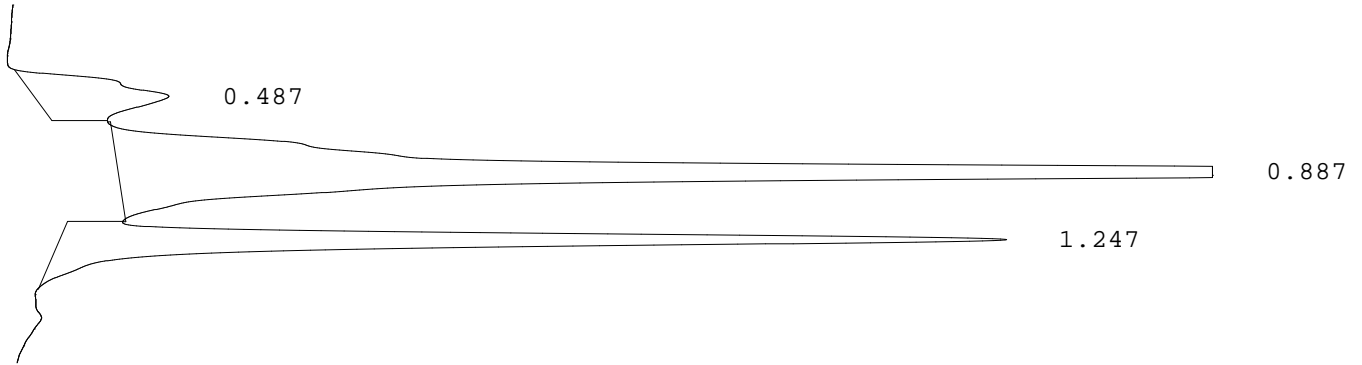

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.487	F 0.55	8.0%	123845	
2	0.887	F 1.00	64.5%	995193	Consistent with F
3	1.247	A 1.00	27.4%	422956	A peak - REVIEW
Total Area: 1541994					

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range